



PCT/GB 2004 / 0 0 4 8 9 5



INVESTOR IN PEOPLE

PRIORITY DOCUMENT
SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH
RULE 17.1(a) OR (b)

The Patent Office
Concept House
Cardiff Road
Newport
South Wales
NP10 8QQ

REC'D 07 JAN 2005

WIPO


PCT

I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.

Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

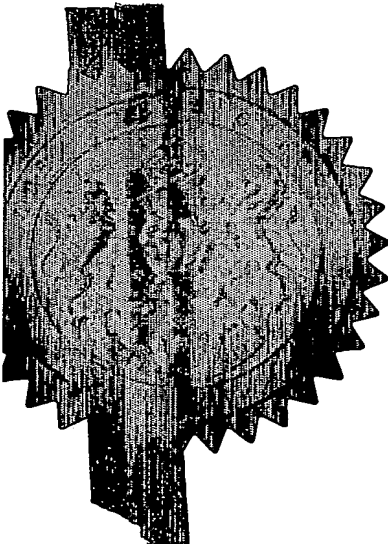

Signed

P. McHoney

Dated

3 December 2004

21 NOV 2003

The
Patent
Office

1/77
21NOV03 E854029-1 001147
P01/7700 0.00-0327112.9

Request for grant of a patent

See notes on the back of this form. You can also get explanatory leaflet from the Patent Office to help fill in this form)

The Patent Office

Cardiff Road
Newport
Gwent NP9 1RH

Your reference

2144

Patent application number

(The Patent Office will fill in this part)

0327112.9

21 NOV 2003

Full name, address and postcode of the or of each applicant (underline all surnames)

Clinical Designs Limited
The Dower House
Aldsworth
Emsworth
Hampshire PO10 8QQ
GB

Patents ADP number (if you know it)

If the applicant is a corporate body, give the country/state of its incorporation

875803900/
GB

Title of the invention

Dispenser and Reservoir

Name of your agent (if you have one)

NIGEL BROOKS CPA

"Address for service" in the United Kingdom to which all correspondence should be sent (including the postcode)

HILL HAMPTON
EAST MEON
PETERSFIELD
HAMPSHIRE GU32 1QN

Patents ADP number (if you know it)

463001/

If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and (if you know it) the or each application number

Country

Priority application number
(if you know it)

Date of filing
(day / month / year)

GB

NA

NA

NA

NA

If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application

Number of earlier application

Date of filing
(day / month / year)

Is a statement of inventorship and of right to grant of a patent required in support of this request? (Answer 'Yes' if:

- a) any applicant named in part 3 is not an inventor, or
 - b) there is an inventor who is not named as an applicant, or
 - c) any named applicant is a corporate body.
- See note (d))

yes

Patents Form 1/77

Enter the number of sheets for any of the following items you are filing with this form.
Do not count copies of the same document

Continuation sheets of this form	0
Description	6 ✓
Claim(s)	0
Abstract	0
Drawing(s)	3 + 3 92

If you are also filing any of the following, state how many against each item.

Priority documents	0
Translations of priority documents	0
Statement of inventorship and right to grant of a patent (Patents Form 7/77)	0
Request for preliminary examination and search (Patents Form 9/77)	0
Request for substantive examination (Patents Form 10/77)	0
Any other documents (please specify)	

I/We request the grant of a patent on the basis of this application.

Signature

Date

20/11/03

Name and daytime telephone number of person to contact in the United Kingdom

NIGEL BROOKS CPA (01730) 823647

Warning

After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.

Notes

If you need help to fill in this form or you have any questions, please contact the Patent Office on 0645 500505.

Write your answers in capital letters using black ink or you may type them.

If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.

If you have answered "Yes" Patents Form 7/77 will need to be filed.

Once you have filled in the form you must remember to sign and date it.

For details of the fee and ways to pay please contact the Patent Office.

DISPENSER and RESERVOIR

The present invention relates to a dispenser, particularly though not exclusively for dispensing aerosol or powder borne medicaments, and to a source
5 reservoir for such a dispenser.

I have applied for a number of patents on dispensers for a gaseous, gas borne or droplet substance. In particular, in my prior International Patent Application, PCT/GB98/00770, at least as amended on entry in the European Regional Phase, there
10 is described and claimed:

A dispenser for a gaseous, gas borne or droplet substance, the dispenser including:

- a body having a mouthpiece with an inhalation/insufflation orifice at its end;
- a junction in the body for a source of gas or evaporable liquid comprising or
15 containing the said substance (the source being carried by the body); and
- a breath actuatable valve, for controlling the release of said gas or liquid, comprising:
 - a valve inlet connected to the junction;
 - a valve outlet;
 - a flexible tube extending from the junction, between the inlet and the outlet, for
20 receiving the said gas or liquid, the tube having a portion which is movable between a closed position in which the tube is kinked for closure of the valve and an open position in which the tube is un-kinked for opening of the valve; and
 - a movable member, for moving the movable portion of the tube to control its
25 kinking, and being movably mounted in the body for movement by the act of inhalation from a rest position towards the orifice – or at least in the direction of air flow through the dispenser;
 - the tube being kinked to an obturating extent when the movable member is in a
30 rest position and un-kinked when the movable member is moved on inhalation for release of the gas or liquid.

Such a dispenser can loosely be classed as a breath actuated, kink valve dispenser and is referred to herein as "My Earlier Breath Actuated, Kink Valve Dispenser".

5 With such a dispenser, in common with others of my design and other designs, there is advantage to the user in knowing how many doses are left in the reservoir of the substance source, the reservoir typically being an aerosol valve can, the can being an aluminium pressing.

10 Two approaches to dose measurement are known.

Firstly, dispensers actuated by depression of the end of the can towards the body of the dispenser body can be provided with electronic or mechanical counters which sense the number of depressions and count down to indicate exhaustion of the
15 dispenser. This approach is costly.

A second approach is to provide the source with a transparent reservoir, typically of glass. Existing glass reservoirs have replicated the shape of the prior pressed aluminium can. Their shape renders difficult estimation of the number of
20 doses remaining.

The object of the present invention is to provide dispenser having a reservoir whose content can be readily estimate, particularly as it approaches exhaustion.

25 According to one aspect of the invention there is provided a dispenser for a gaseous, gas borne or droplet substance having a source of the substance, the source having a reservoir with:

- a major portion having a comparatively large cross-section of its substance space and
- 30 • a minor portion having a comparatively small cross-section of its substance space,

the reservoir being translucent, and preferably transparent, at the minor portion at least, whereby a user can note a comparatively rapid depletion with use of the

quantity of substance remaining when the source approaches exhaustion of the substance.

According to a second aspect of the invention there is provided a source for a dispenser of a gaseous, gas borne or droplet substance from the source, the source having a reservoir with:

- a major portion having a comparatively large cross-section of its substance space and
- a minor portion having a comparatively small cross-section of its substance space,

the reservoir being translucent, and preferably transparent, at the minor portion at least, whereby a user can note a comparatively rapid depletion with use of the quantity of substance remaining when the source approaches exhaustion of the substance.

According to a third aspect of the invention there is provided a reservoir for a source of a gaseous, gas borne or droplet substance to be used in a dispenser, the reservoir having:

- a major portion having a comparatively large cross-section of its substance space and
- a minor portion having a comparatively small cross-section of its substance space,

the reservoir being translucent, and preferably transparent, at the minor portion at least, whereby a user can note a comparatively rapid depletion with use of the quantity of substance remaining when the source approaches exhaustion of the substance.

The minor portion can have a constant cross-section or a progressively diminishing cross-section, whereby the rate of fall of the level of the substance increases as it is further depleted.

Normally the minor portion will be at the opposite end of the source from its release valve, with the user holding the dispenser valve-up to observe the level of the

substance in the minor portion. However, the minor portion could be provided at the valve end of the reservoir as a diminishing cross-section neck.

The reservoir can be of glass or transparent/translucent plastics material.

5 Where it is of glass, this can be enclosed in a plastics material sheath, typically a shrink wrapping or an insert moulding, i.e. a moulding of the plastics material sheath onto the glass reservoir within a mould tool. Where the minor portion is to have a cross-section so small as to be impractical to form in glass, in production with sufficient precision, it is envisaged that the reservoir as such can be provided as a
10 plastics material moulding, possibly enclosed by a robust, impermeable outer enclosure, such as a glass casing, itself enclosed in a shrink wrapping or an insert moulding for instance.

Alternatively, the reservoir can be provided with an insert, which substantially
15 reduces the cross-section thereof, typically at its end distal from the valve. Again, the insert can be at the valve end. In either case the insert can be formed as part of a component of the valve in the source for metering a dose from its reservoir. The insert can be parallel or tapered, the latter shape providing an increasing rate of fall with depletion.

20

To help understanding of the invention, various specific embodiments thereof will now be described by way of example and with reference to the accompanying drawings, in which:

Figure 1 is a side view of a dispenser according to the invention;

25 Figure 2 is a scrap view of the reservoir of the dispenser of Figure 1, inverted and approaching depletion;

Figure 3 is a view similar to Figure 1 of another dispenser of the invention;
and

Figure 4 is a similar view of a third dispenser of the invention.

30

Referring to Figure 1, the dispenser 1 has a source 2 of medicament with a transparent reservoir 3 of glass sheathed in a transparent plastics material shrink wrapping 4, which provides an enclosure against explosion of the glass in the event of

accidental breakage of the glass. The reservoir contains not only a liquid medicament 5, but also a gaseous propellant liable to cause the glass to explode if broken.

5 A valve 6 of the source, shown only in outline in Figure 1, is within a body 7 of the dispenser. The valve is attached to the reservoir by a crimped-on aluminium sleeve 8.

10 The reservoir is parallel 11 through much of its length, where it has a comparatively large cross-section of its substance space 12, but has a tapered tip 13 remote from the valve 6, where it has a comparatively smaller and decreasing cross-section.

15 With the dispenser inverted, Figure 2, the level 14 of the medicament 5 is within the tapered tip when the medicament is close to being used up. As use of the dispenser continues, the level falls progressively faster, giving the user an indication that a fresh dispenser will soon be required. Typically the user will take a fresh dispenser with him when the level is such as to indicate that the daily number of doses will exhaust the reservoir.

20 Turning to Figure 3, the dispenser 101 there shown has a glass reservoir 103 within a welded-on transparent cover 121, welded at a position appropriate for its breath actuated, kink valve mechanism, such as disclosed in my patent application No. PCT/GB03/001102. The reservoir has indents 122 in the glass which provides dimples 123 on the inside surface of the reservoir. An opaque plastics material slug 25 124 is pushed past the dimples, to be held by the dimple against an end 125 of the reservoir. The slug has a ribs 126 keeping it centred in the reservoir and a diameter such that the peripheral space between the slug and the inner wall of the reservoir has a considerably reduced cross-section in comparison with that of the reservoir where the slug is not present.

30

As the source approaches exhaustion, the level observed in the reservoir when inverted drops to be in slug/glass annulus 127. As in the Figure 1 embodiment, this gives a good indication of impending exhaustion.

Turning now to Figure 4, the dispenser 201 there shown again has a parallel glass reservoir 203. Within it is a translucent plastics material lining of a shape essentially similar to that of the reservoir 3, i.e. with a tip 213 of lesser cross-section. The exhaustion level can be observed in this also.

1/3

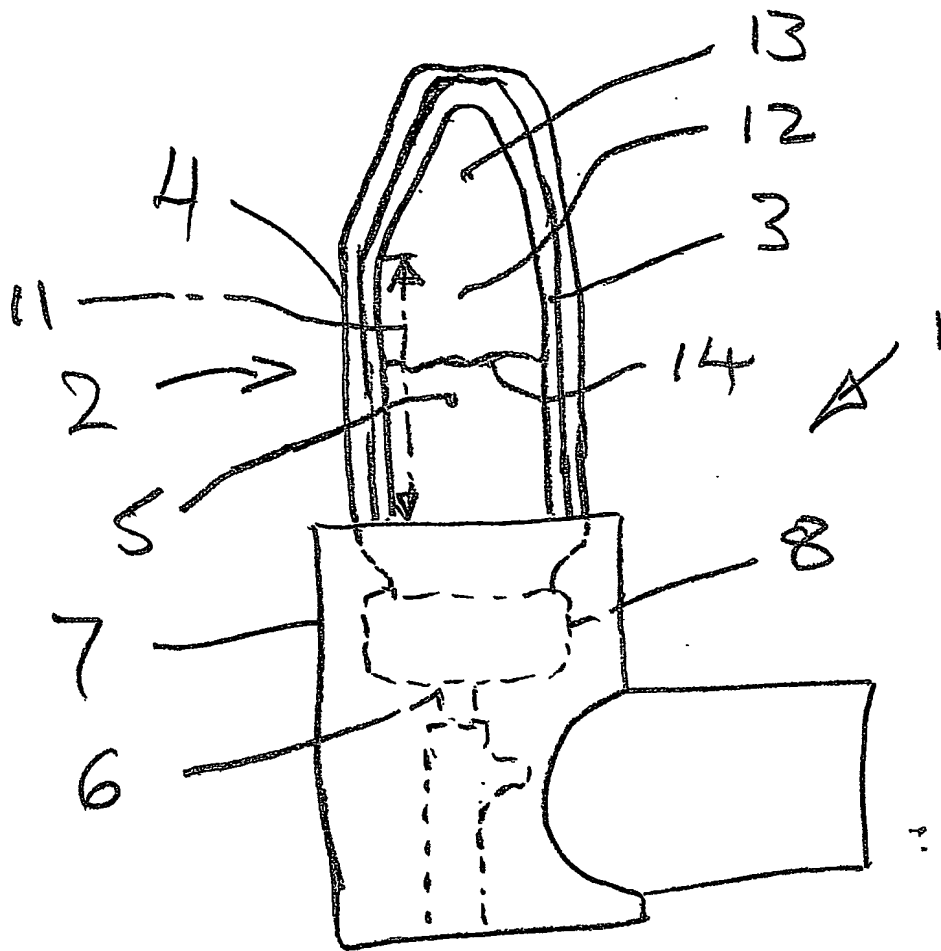


FIGURE 1

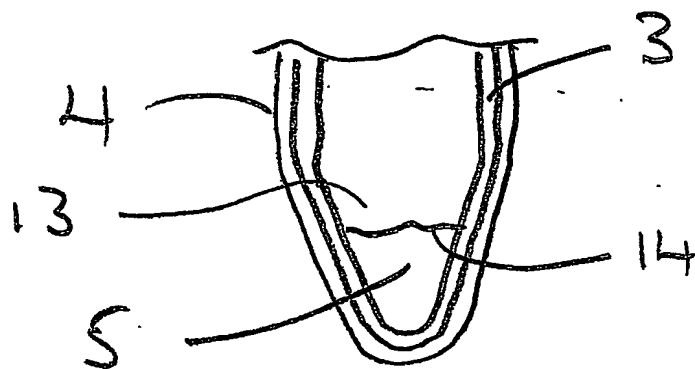


FIGURE 2

2/3

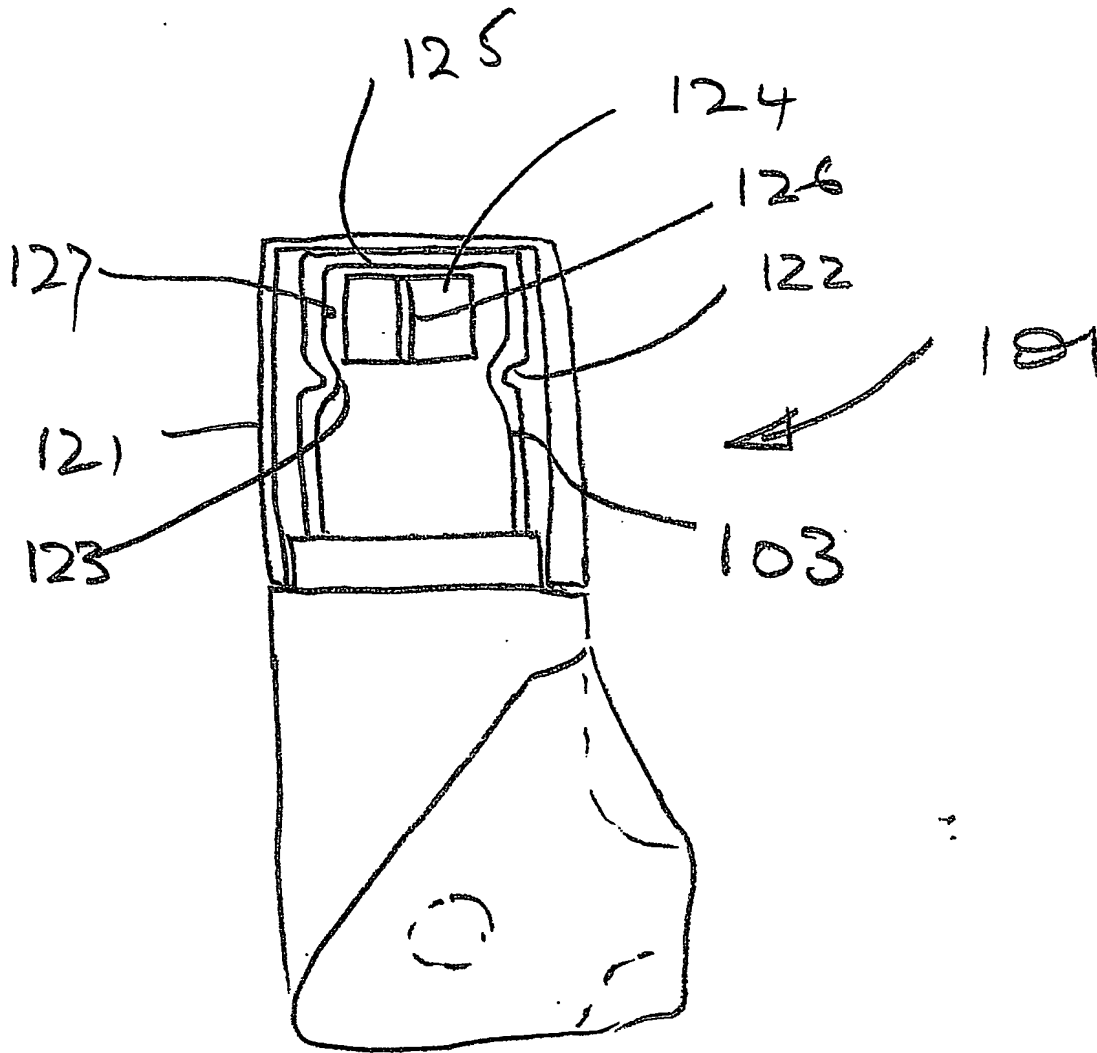


FIGURE 3

3/3

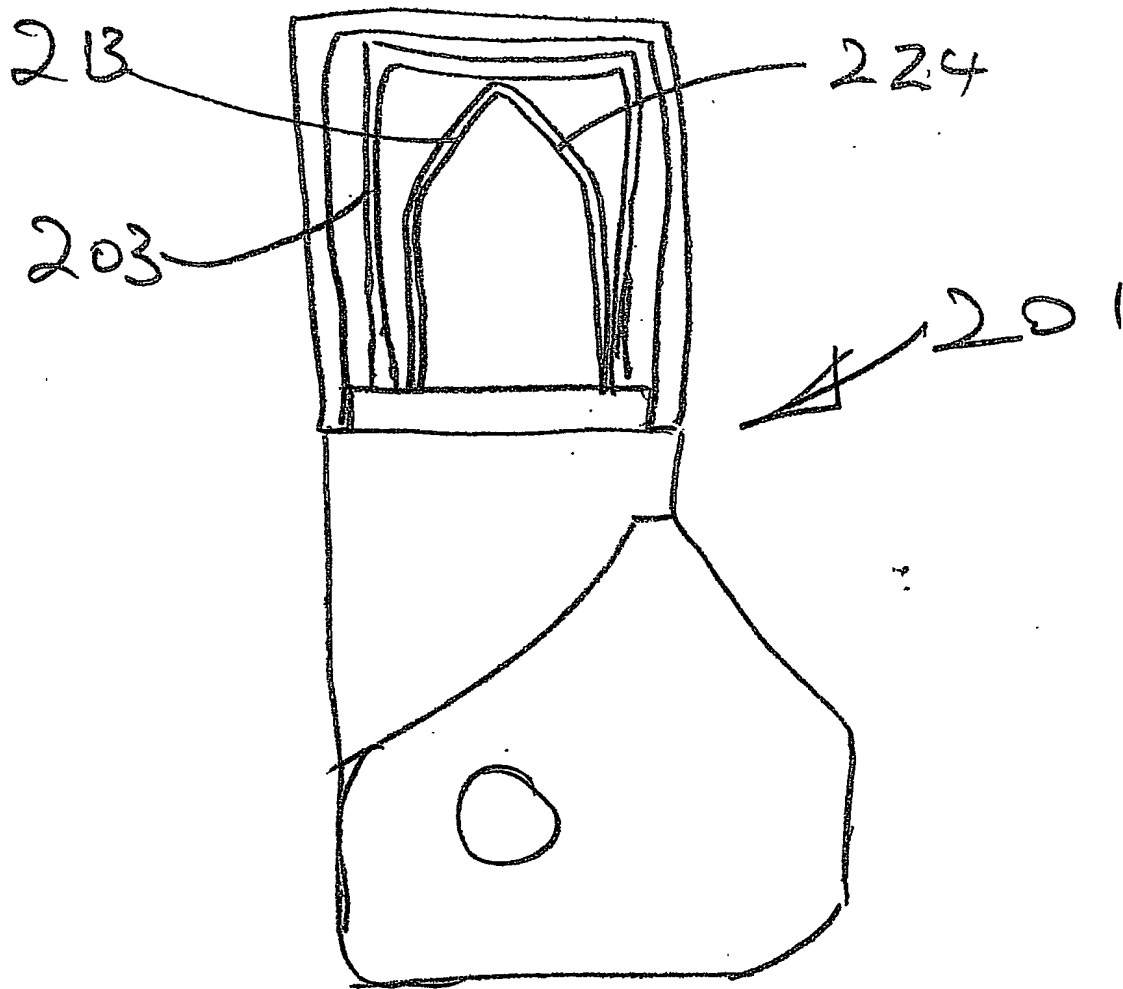


FIGURE 4

This Page is Inserted by IFW Indexing and Scanning Operations and is not part of the Official Record.

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☒ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☒ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☒ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.